


# Pediatric Pulse™ Algorithm

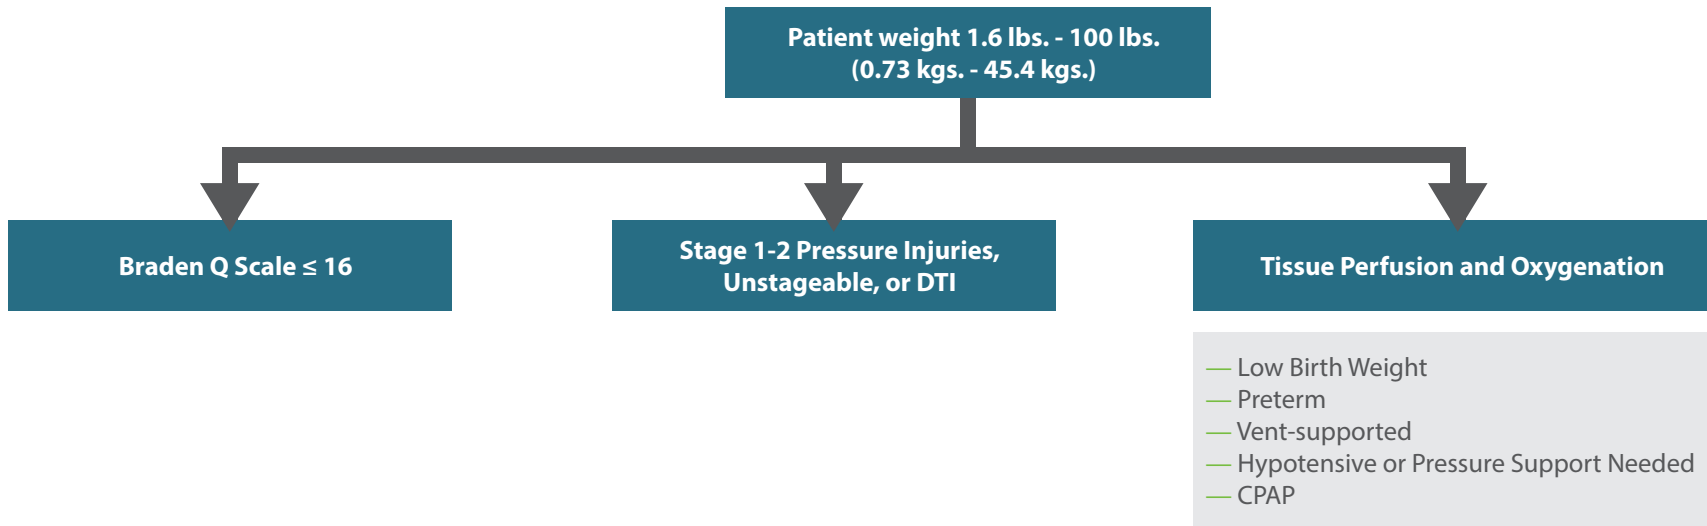

## Note:

Pediatric Pulse measures feedback pressure that is optimized with a patient weight of at least 1.6 lbs./0.73 kgs.

## Contraindications:

- If > 100 lbs./45.4 kgs.
- If < 1.6 lbs./0.73 kgs.
- Unstable Spine



## Pediatric Pulse™

- 100 lbs. capacity
- Adjustable pulsation cycle: 3-20 minutes
- Passive massage action to aid in the increase of capillary blood flow
- Lockout controls
- Power failure/Low pressure audible and visual alarms
- Vapor-permeable, low-friction, and anti-shear top cover
- Customized to fit virtually any hospital crib

## References:

Schumacher, B., Askew, M., and Otten (2012). Development of a pressure ulcer trigger tool for the neonatal population. *Journal of Wound, Ostomy and Continence*, 39(6), 1-5.  
Noonan, C., Quigley, S., and Curley, M.A.Q. (2011). Using the Braden Q Scale to Predict Pressure Ulcer Risk in Pediatric Patients. *Journal of Pediatric Nursing*, 26(6), 566-575.

**Learn more: Call 800-814-9389**  
or contact your Sizewise rep